
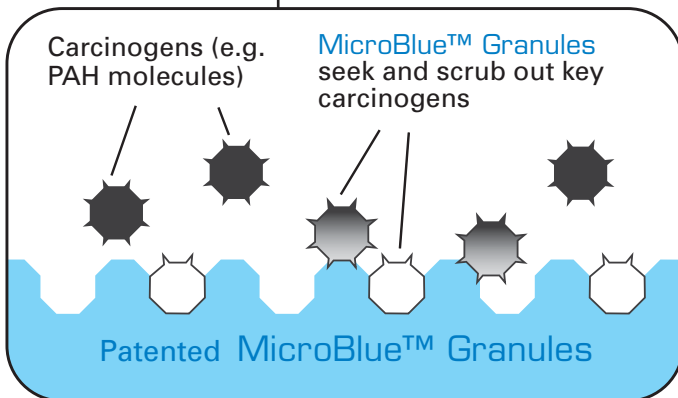


# MicroBlue™ BlueTip

## Cigarette Holder

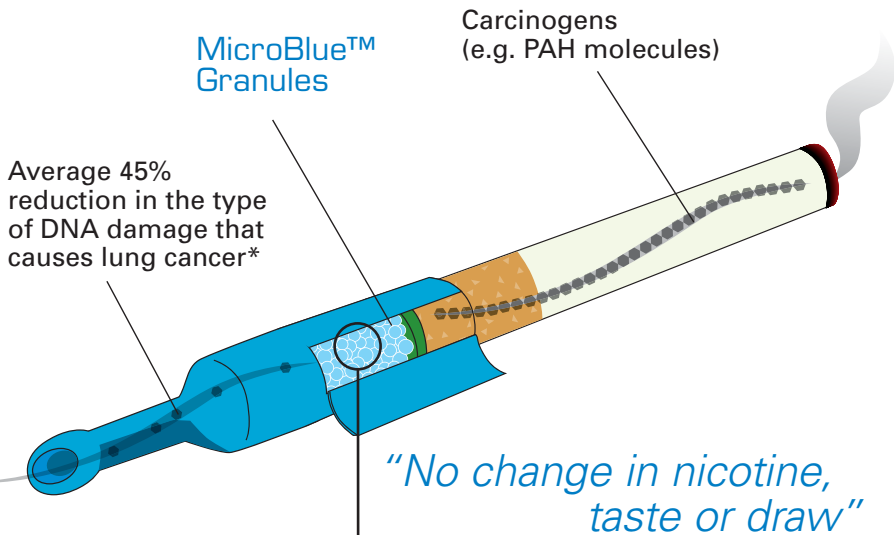

*artistic representation only*

\* Toxicity reduction based on measurement of base-pair DNA mutations (Ames Test TA-100/+S9), achieved in Gen 4 filter tests